



Inhibitory Effect of Gallium Nitrate against *Staphylococcus aureus* and Its Action on the Formation of Biofilms on Titanium Surfaces

Amanda Stefanie Jabur de Assis^{a*},
Guilherme Manassés Pegoraro^a, Tais Germano-Costa^b,
Renata de Lima^b, Natan de Jesus Pimentel-Filho^c
and Iolanda Cristina Silveira Duarte^b

^a Center of Science and Technology for Sustainability (CCTS), Federal University of São Carlos (UFSCar), Sorocaba, SP, Brazil.

^b LABiToN (Laboratory of Bioactivity Assessment and Toxicology of Nanomaterials), University of Sorocaba, SP, Brazil.

^c Center for Natural Sciences, Federal University of São Carlos (UFSCar), Buri, SP, Brazil.

Authors' contributions

This work was carried out in collaboration among all authors. All authors read and approved the final manuscript.

Article Information

DOI: 10.9734/BJI/2023/v27i2675

Open Peer Review History:

This journal follows the Advanced Open Peer Review policy. Identity of the Reviewers, Editor(s) and additional Reviewers, peer review comments, different versions of the manuscript, comments of the editors, etc are available here: <https://www.sdiarticle5.com/review-history/99020>

Original Research Article

Received: 18/02/2023

Accepted: 22/04/2023

Published: 26/04/2023

ABSTRACT

Aims: This study aimed to investigate the effect of gallium nitrate [Ga(NO₃)₃], an inorganic antimicrobial agent, against the growth and biofilm formation of *Staphylococcus aureus* on the titanium surface.

*Corresponding author: E-mail: amanda.jabur@gmail.com;

Study Design: This study is a laboratory investigation involving the determination of the inhibitory concentration (IC) of $\text{Ga}(\text{NO}_3)_3$ against the planktonic strain of *S. aureus* and biofilm formation on titanium coupons.

Place and Duration of Study: Sample: Center of Science and Technology for Sustainability (CCTS), Federal University of São Carlos, SP, Brazil, between March 2020 and March 2022.

Methodology: The inhibitory concentration of gallium nitrate was determined in a 96-well microtiter plate in Muller Hinton broth. The potential of the antimicrobial agent to inhibit biofilm formation by *S. aureus* on titanium surfaces was evaluated by Scanning Electron Microscopy (SEM). The cytotoxicity potential of $\text{Ga}(\text{NO}_3)_3$ was determined on V79 cells.

Results: The results showed that the susceptibility of gallium nitrate against *S. aureus* was 1.40 μM , while SEM images revealed that concentrations of 90 μM inhibited biofilm formation by *S. aureus*.

Conclusion: This research has shown promising results regarding gallium nitrate's potential of inhibiting the growth of both planktonic and sessile *S. aureus* cells. In addition, coating titanium surfaces with $\text{Ga}(\text{NO}_3)_3$ would be an extra alternative to prevent implant-associated infections due to its non-toxicity to cells.

Keywords: Antimicrobial; biofilms; gallium nitrate; *Staphylococcus aureus*; titanium.

1. INTRODUCTION

Despite being considered a Gram-positive opportunistic pathogen, *Staphylococcus aureus* is found in both the environment and as part of the human microbiota, colonizing the skin and nasal mucosa of healthy individuals [1]. The strains cross the border of pathogenicity when entering the bloodstream or internal tissues, causing a wide variety of infections. As its reproduction can occur aerobically and anaerobically at temperatures ranging from 18 to 40 °C, several clinical manifestations are favored by these conditions [2,3].

The areas most affected by *S. aureus* include skin and soft tissues, originating infections such as folliculitis, bacteremia, and pneumonia. In addition, medical devices are also impacted by these bacteria, due to their versatility when found in different hosts and environments or for being capable of withstanding a wide range of temperatures [1,4].

For decades, titanium devices have been reported as a product of successful prosthetic rehabilitation and dental implants based on their biocompatibility and stability. However, despite the prosperous rise of these instruments, they were also found to exhibit biofilm-associated infections [5]. In the past, the risk of failure in these titanium-based instruments was still considered significant, as a result of incompatibility between tissue and biomaterial, surgical trauma, and material imperfections. However, while these barriers were overcome, another issue arose: the emergence of bacterial

infections - a contemporary problem with yet no clear solution [6].

In order to prevent infections associated with bacterial biofilms on titanium devices, surface modification, and chemical element deposition have been reported, avoiding bacterial colonization. The association of silver, zinc, copper, or gallium ions with titanium surfaces produced inhibitory effects against biofilms [7,8, 9, Petrini et al.,2006; 10].

As a result of its toxicity to bacteria, antimicrobial metal compounds containing gallium (Ga^{3+}) – a transition metal element from group 13 of the periodic table with relevant chemical properties that are similar to Fe^{3+} – make it a pioneering antimicrobial agent, by interfering with iron regulation in microorganisms. Primordial bacterial activities such as metabolism, cellular respiration, and DNA synthesis are Fe^{3+} dependent, so the Ga^{3+} strategy relies on its mimicry to “trick” the Fe^{3+} receptors and enter the cell [11,12]. In the cell, Ga^{3+} cannot be functional, resulting in disruptions in the microorganisms' metabolism.

In this work, we aimed to explore the antimicrobial effect in order to determine the inhibitory concentration of gallium nitrate in solution against the common bacterial strain reported in titanium device infections: *S. aureus*. Meanwhile, cytotoxicity tests in cells were performed, and scanning electron microscopy (SEM) was chosen to evaluate the biofilm inhibition by $\text{Ga}(\text{NO}_3)_3$.

2. MATERIALS AND METHODS

2.1 Chemicals, Microbial Strain, and Culture Conditions

Staphylococcus aureus ATCC 6538 was cultivated under anaerobic conditions at 37°C for 18 h in Tryptic Soy Agar (TSA). In the susceptibility test, *S. aureus* was grown aerobically at 37°C in Mueller-Hinton Broth (MHB; Difco™, USA) in a 96-well microplate.

The analysed gallium compound, Ga(NO₃)₃·xH₂O (crystalline, 99.9% trace metals basis; Sigma-Aldrich®, USA), was dissolved in 1.0 M sodium citrate [(CH₂COONa)₂·2H₂O] buffer.

Initially, when gallium nitrate was diluted in water, the pH of the solution decreased to the range of 2.3 – 2.5 and there was a change in the turbidity caused by the formation of a precipitate that interfered with the spectrometric measurements. Thus, to reduce these variations, especially at higher concentrations, Ga(NO₃)₃ was diluted in 1.0 M sodium citrate buffer, and pH was adjusted between 7.0 and 8.0 in order to reduce turbidity.

2.2 Susceptibility Testing

In order to determine the inhibitory concentration (IC) of Ga(NO₃)₃, 200 µL of MHB supplemented with gallium nitrate at concentrations ranging from 0.17 to 90 µM were transferred to 96-well microplates and inoculated with approximately 10⁷ cfu/mL of *S. aureus* ATCC 6538 previously grown in the same broth. According to Xu et al., 2017, the Ga(NO₃)₃ solution has a few flocs at higher concentrations, so 10 µL of 0.2 % EDTA solution was added to each well in order to eliminate any interference with the absorbance reading.

Afterward, the microplate was incubated for 24 h at 35 °C and read at 540 nm with a microplate reader (Synergy HTX Multimode Reader, Brazil).

2.3 Effect of Ga(NO₃)₃ on Biofilm Formation by *S. aureus* on Titanium Surfaces

Titanium coupons (10 × 10 mm, 2 mm in thickness, grade II) were polished with #100, #300, #500, and #800 grit SiC abrasive papers. Subsequently, the coupons were washed with liquid-neutral detergent and water, followed by rinsing with distilled water and then immersing in

70 % ethyl alcohol for 1 h to remove fat. The titanium coupons were then rinsed again with distilled water and air-dried under UV light. The cleaned coupons were immersed for 18 h at 37°C in MHB supplemented with 90 µM of Ga(NO₃)₃ without bacteria-denominated negative control; in MHB with approximately 1 × 10⁷ CFU/mL of exponentially growing *S. aureus* cells (optical density at 600nm [OD₆₀₀] of 0.2) – named positive control; and in MHB supplemented with 90 µM Ga(NO₃)₃ containing growing cells – denominated treatment.

To evaluate the inhibition effect of gallium nitrate on the biofilm formation, the titanium coupons were rinsed in sterile distilled water after incubation, dried under laminar airflow, and observed via SEM imaging at 300x and 1500x magnification (JEOL – JSM-IT200A, Brazil). Cleaned and sanitized coupons also were observed by SEM.

2.4 Cytotoxicity Evaluation

To evaluate the cytotoxic potential of gallium nitrate, normal Hamster lung cells (V79 lineage) were used. Cells were plated at a concentration of 1 × 10⁵ cells/well in 96-well plates and incubated at 37°C under 5 % CO₂. After 24 h, the cells fully adhered to the polystyrene surface and were exposed to Ga(NO₃)₃. The exposure was carried out under increasing concentrations of gallium nitrate, ranging from 39.10 to 273.71 µM, for a period of 24 h at 37°C under 5 % CO₂. After incubation, Ga(NO₃)₃ solution was removed from the culture, and the cells were washed with phosphate-buffered saline (PBS). Then, 100 µL of 3-(4,5-dimethyl thiazolyl-2)-2,5-diphenyltetrazolium bromide solution (MTT) at a concentration of 0.5 mg/mL (v/v) were added to each well and the plate was incubated again for 3 h at 37°C under 5 % CO₂. Finally, the MTT solution was removed, and for cell fixation, 100 µL of dimethyl sulfoxide (DMSO) was added to each well. Cell viability analysis was performed using the microplate reading equipment (RCHISTO Tecan Infinite®, Brazil) at a wavelength of 570 nm.

2.5 Statistics

Statistical analysis employed a one-way analysis of variance (ANOVA) followed by Tukey's test (significance level of $p=0.05$), performed using OriginPro 2021b 9.85v.

3. RESULTS

3.1 Effect of $\text{Ga}(\text{NO}_3)_3$ on the Growth of *S. aureus*

The inhibitory concentration of gallium nitrate against *S. aureus* ATCC 6538 was investigated in MHB. In higher concentrations, the $\text{Ga}(\text{NO}_3)_3$ precipitation during cultivation interfered with absorbance measurements avoiding the correct determination of the inhibitory concentration (Fig. 1). However, the study still revealed that the inhibitory concentration was able to inhibit 50 % of the strain when compared to the absorbance results of the pathogen's positive control ($p=0.05$). The negative control, MHB supplemented with only $\text{Ga}(\text{NO}_3)_3$, did not show any interference with the absorbance. The results showed an inhibition effect of gallium nitrate at 1.40 μM against *S. aureus* (Fig. 1).

3.2 Biofilm Inhibition

Scanning electron microscopy was used to evaluate the ability of *S. aureus* to form biofilms on titanium surfaces in the absence and presence of gallium nitrate. The uniformity of the cleaned and sanitized titanium coupon surfaces

is presented in Figs. 2A and Fig. 2B, at 300x and 1500x magnification, respectively. Figs. 2C and 2D show the titanium surfaces under the same magnifications after its immersion in MHB supplemented with $\text{Ga}(\text{NO}_3)_3$ for 18 h. The positive control is shown in Figs. 2E and 2F, which represent *S. aureus*' typical biofilm structure.

When titanium coupons were immersed in MHB supplemented with 90 μM of gallium nitrate and inoculated with *S. aureus*, no typical biofilm structure was observed (Fig. 2G and 2H). The topography noted in the images is characteristic of the microstructure of gallium adsorbed on the metal surface.

3.3 Cytotoxic Effect of $\text{Ga}(\text{NO}_3)_3$ in Cell Lines

The cytotoxicity of gallium nitrate was evaluated on V79 cells. The MTT assay revealed low cytotoxicity for all tested concentrations of $\text{Ga}(\text{NO}_3)_3$ (Fig. 3), indicating that the antimicrobial agent does not inhibit the growth of healthy cells, acting only against pathogenic ones.

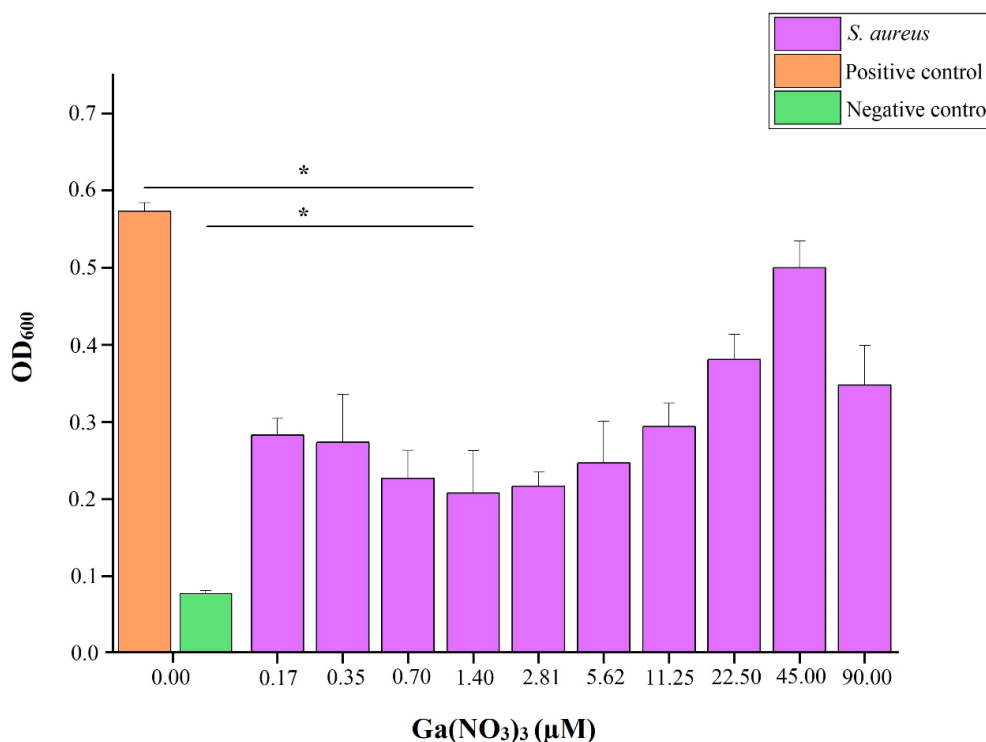


Fig. 1. Susceptibility of *S. aureus* treated with $\text{Ga}(\text{NO}_3)_3$. Statistical significance between the absorbances data of positive and negative control against the pathogen data is indicated by an asterisk (* $P=0.05$)

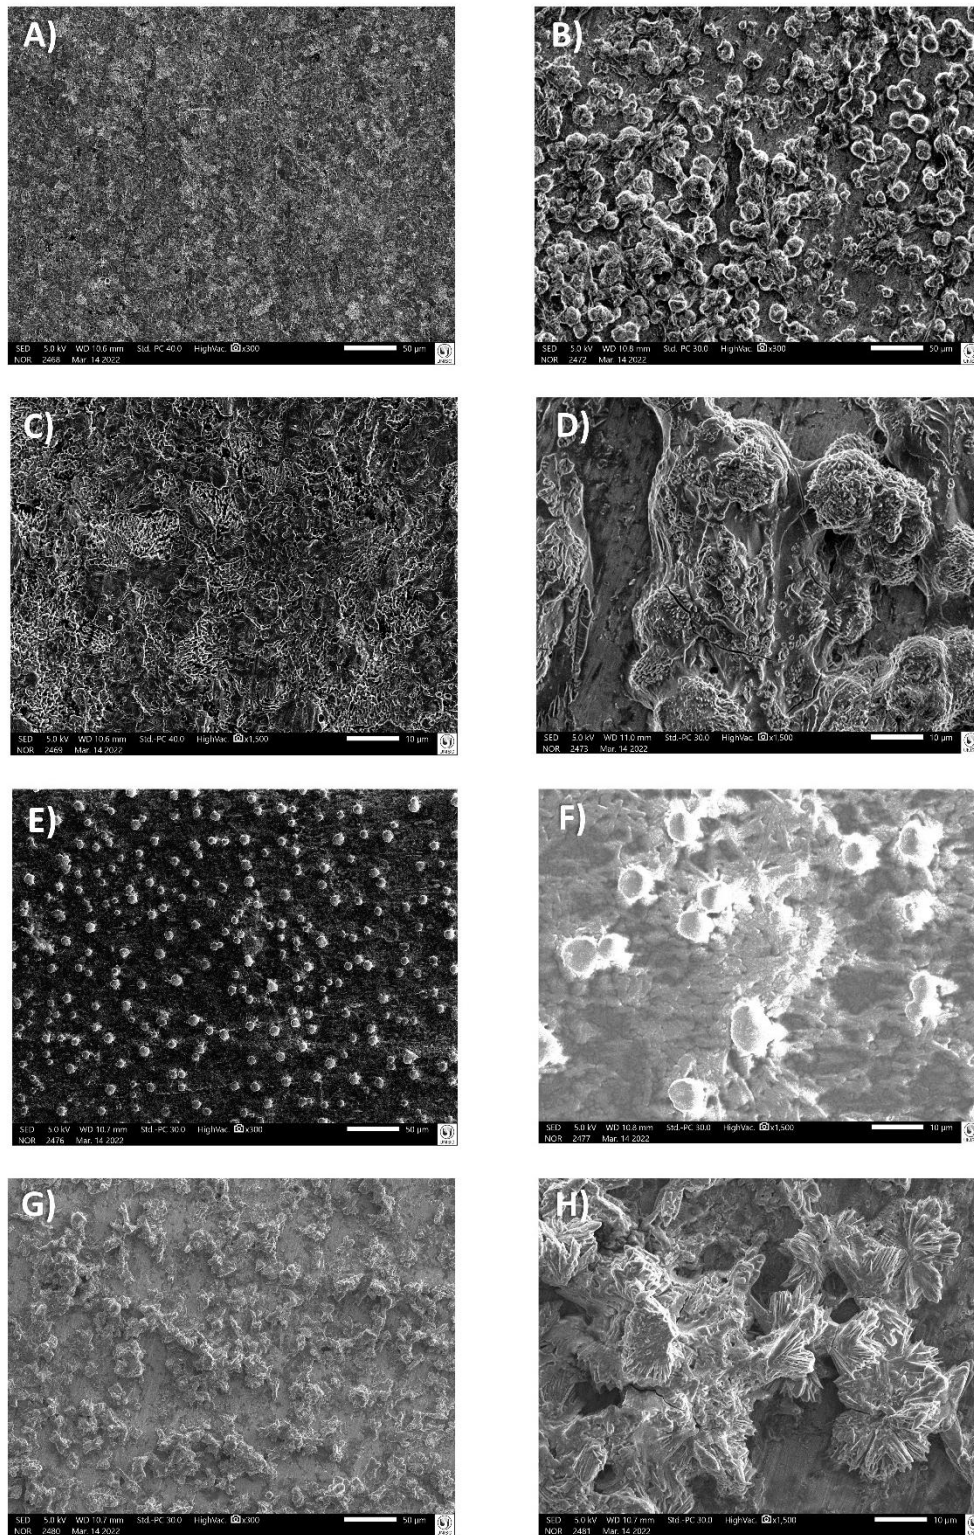


Fig. 2. Scanning electron microscopy of *S. aureus* biofilm on titanium surfaces in the presence and absence of $\text{Ga}(\text{NO}_3)_3$. Images were captured for a clean and sanitized titanium coupon (A and B), a titanium coupon treated with MHB supplemented $\text{Ga}(\text{NO}_3)_3$ (C and D), a titanium coupon immersed in MHB with the addition of *S. aureus* (E and F), and a titanium coupon immersed in MHB supplemented with $\text{Ga}(\text{NO}_3)_3$ with the addition of *S. aureus* (G and H). Two resolutions were used to obtain the images: 300x (A, C, E, and G) and 1500x (B, D, F, and H)

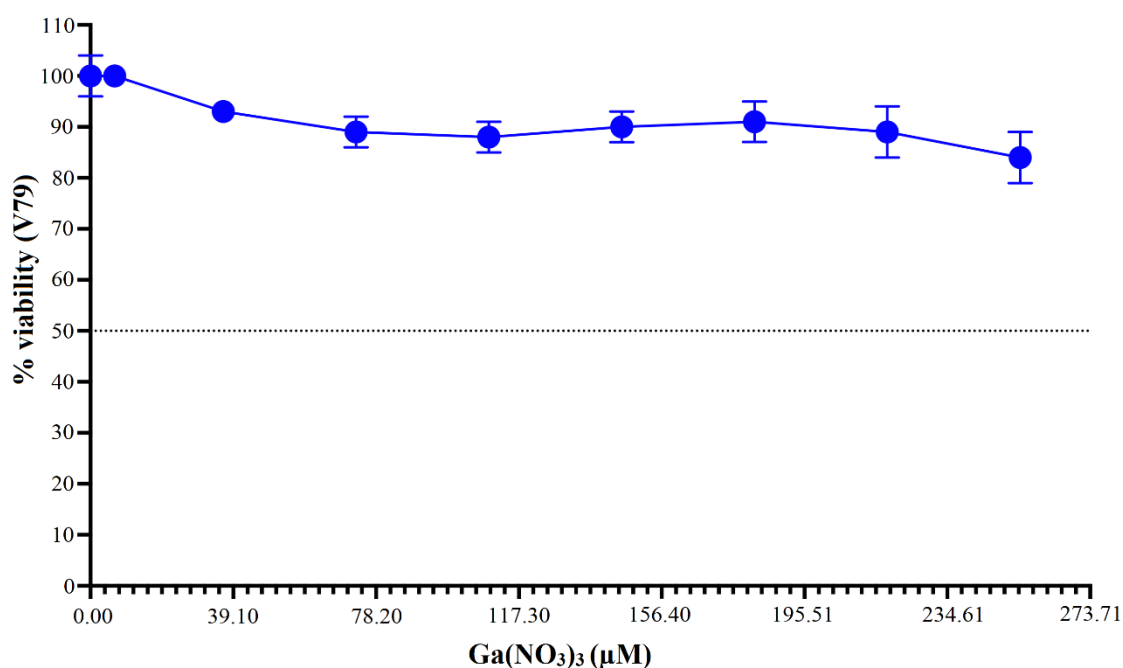


Fig. 3. V79 lineage cell viability in the presence of different concentrations of Ga(NO₃)₃.

4. DISCUSSION

Among metallic ions, Ga³⁺ stands out for being an antimicrobial agent that acts against several targets, in addition to being able to bind to iron-dependent proteins to enter the cell as a “Trojan Horse” and cause an interruption in the enzymatic metabolism of the microorganism [13, 14]. Therefore, due to the increase in arthroplasty and infections associated with these devices by multidrug-resistant microorganisms, such as *S. aureus*, gallium nitrate was used to inhibit planktonic growth and biofilm formation by this important opportunistic pathogen on titanium-based surfaces.

However, after the dilution of gallium nitrate in aqueous medium, a complex began to precipitate, interfering with the turbidity of the solution and causing the acidification of the medium, as previously reported by Tsukatania et al. [15]. According to Zhao et al. [16], the precipitate in this type of solution corresponds to Ga(OH)₃. When Ga(NO₃)₃ is added to aqueous solutions, gallium ions react with OH⁻ ions, which results in the precipitate formation, identified as gallium hydroxide [Ga(OH)₃] [17]. In order to avoid this phenomenon, Ga(NO₃)₃ was diluted in sodium citrate solution. There was minimal change in the turbidity even following pH adjustment to neutral values with NaOH. This circumstance corroborates with Rzepishevskaya et

al. (2011), who reported the use of gallium citrate (Ga-Cit) in order to prevent precipitation of Ga(OH)₃, allowing the investigation of the minimum inhibitory concentration of gallium nitrate against Gram-negative and Gram-positive planktonic bacteria with minor interference.

Despite the buffer solution supplemented with Ga(NO₃)₃ not being fully effective in the control of *S. aureus* ATCC 6538 (Fig. 1), for the evaluated concentrations, the results still proved it to be an efficient antimicrobial agent against the pathogen. The required inhibitory concentration to inhibit 50% of *S. aureus* cells was 1.40 µM. This concentration of the antimicrobial, expressed in micromolar, reduced the absorbance by 50% when compared to that found in the positive control.

It was also possible to notice that the Gram-positive *S. aureus* was sensitive to gallium nitrate, which can be attributed to the presence of only one barrier preventing access to the cytoplasm in Gram-positive strains, resulting in lower required concentrations of the antimicrobial agent. This evidence corroborates those established in the literature. Garcia et al. [18] studied the action of poly(methyl methacrylate) (PMMA) and calcium sulfate (CaSO₄), which are compounds frequently used in the treatment of orthopedic infections involving strains of *Staphylococcus* spp., by delivering Ga(NO₃)₃ to

infected sites. In addition, the complex's effectiveness as an antimicrobial agent against strains of *S. aureus* and *Staphylococcus epidermidis* was evaluated [18]. As a result, data revealed a significant decrease in microbial growth at concentrations above 16 μM and 4 μM , respectively, while concentrations above 64 μM completely inhibited both trialed strains. In our current work, concentrations of 90 μM were found to completely inhibit biofilm formation on titanium surfaces, values similar to those found by Garcia et al. [18], who observed the inhibition of *S. aureus* biofilms in the presence of concentrations above 128 μM .

In 2017, Dong et al. [19] tested the inhibitory effect of $\text{Ga}(\text{NO}_3)_3$ on *Pseudomonas aeruginosa* and *S. aureus* biofilms on titanium chips. A thin layer of gallium nitrate was used, which was found to be effective against the *P. aeruginosa* strain, but the results against *S. aureus* were negligible. The need for high concentrations of $\text{Ga}(\text{NO}_3)_3$ was demonstrated in recent studies. Gugala et al. [20] evaluated the effectiveness of the antimicrobial on isolated species of *Escherichia coli*, *P. aeruginosa*, and *S. aureus*. They have found a minimal inhibitory concentration of gallium nitrate against these strains, which needed 31,250 μM , 15,630 μM , and 15,620 μM , respectively [20]. On the other hand, the effectiveness of much lower concentrations of $\text{Ga}(\text{NO}_3)_3$ has been demonstrated in the present study, either by inhibiting planktonic growth or by inhibiting the formation of biofilms by *S. aureus* on titanium coupons.

Upon finding the effectiveness of gallium nitrate, cytotoxicity tests were necessary to evaluate the potential to cause damage to healthy mammalian cells. The present study showed that $\text{Ga}(\text{NO}_3)_3$ is not toxic to hamster lung cells (V79 lineage) under concentrations above 39.10 μM . Similarly, in the study conducted by Best et al. [21], three polysaccharides (carboxymethyl cellulose, alginate, and pectin) were tested as binding and delivery agents in three different bacteria (*P. aeruginosa*, *E. coli*, and *S. aureus*) with potential bioresponsive mode. As a result, gallium loaded with carboxymethyl cellulose showed an effective inhibitory activity against all microbial growth and did not exhibit a cytotoxic effect on human dermal neonatal fibroblasts (HDNF) [21]. Rodríguez-Contreras et al. [22] highlight the positive antimicrobial results of Ga^{3+} without inducing cytotoxicity when using it on internal and external titanium surfaces obtained by 3D

printing. The presence of a layer of calcium titanate containing Ga^{3+} adhered to the substrate was revealed. In addition, Ga^{3+} ions promoted the antibacterial effect against Gram-positive strains, especially *P. aeruginosa*, and did not have cytotoxic action against human osteoblasts (SAOS-2) [22]. Cochis et al. [23] investigated the addition of Ga^{3+} ions to titanium alloys, producing intermetallics with high stability and an increase of 1 to 23% gallium in weight. These alloys guaranteed the antibacterial effect without any visible cytotoxic effect, evaluated by direct and indirect contact tests with mature osteoblasts and preosteoblasts progenitor cells [23].

5. CONCLUSION

Our study showed the effect of 1.40 μM of gallium nitrate in reducing the planktonic growth of *S. aureus* by 50 %. Thereby, it was shown that $\text{Ga}(\text{NO}_3)_3$ has an effective role as an antimicrobial agent against biofilms in representative biomaterials used in arthroplasties without visible cytotoxicity under concentrations ranging from 39.10 to 273.71 μM . In addition, besides representing a microbial growth inhibitory tool, gallium nitrate also has the potential to be used in the deposition of biomaterials in order to prevent healthcare-associated infections. In order to advance studies involving medical devices and pathogenic microorganisms, further research is needed, especially regarding the antimicrobial effect of $\text{Ga}(\text{NO}_3)_3$ on other strains commonly found in hospital environments and its involvement in hospital tools.

DISCLAIMER

This paper is an extended version of a preprint document of the same author.

The preprint document is available in this link: <https://www.researchsquare.com/article/rs-2303558/v1>.

[As per journal policy, preprint article can be published as a journal article, provided it is not published in any other journal].

ACKNOWLEDGEMENTS

This study received funding from *Coordination for the Improvement of Higher Education Personnel* (CAPES).

COMPETING INTERESTS

Authors have declared that no competing interests exist.

REFERENCES

1. Tong SYC, Davis JS, Eichenberger E, Holland T, Fowler Jr VG. *Staphylococcus aureus* Infections: Epidemiology, pathophysiology, clinical manifestations, and management. *Clin Microbiol Rev.* 2015;28:603-661.
2. Le KY, Otto M. Quorum-sensing regulation in staphylococci—an overview. *Front. Microbiol.* 2015;6:1174.
3. Rasigade JP, Vandenesch F. *Staphylococcus aureus*: a pathogen with still unresolved issues. *Infect Genet Evol.* 2014;21:510-514.
4. Taylor TA, Unakal CG. *Staphylococcus aureus*. Treasure Island (FL): StatPearls Publishing; 2022.
5. Thukkaram M, Cools P, Nikiforov A, Rigole P, Coenye T, Van Der Voor P. Antibacterial activity of a porous silver doped TiO₂ coating on titanium substrates synthesized by plasma electrolytic oxidation. *J Appl Surf Sci.* 2020;500:1–144235.11.
6. Godoy-Gallardo M, Mas-Moruno C, Fernández-Calderón MC, Pérez-Giraldo C, Manero JM, Albericio F, et al. Covalent immobilization of hLf1-11 peptide on a titanium surface reduces bacterial adhesion and biofilm formation. *Acta Biomater.* 2014;10(8):3522-3534.
7. Dong J, Yang Y, Xiang B, Wang Z, Zhang Y, Huang Y. Study of the Inhibitory effect of gallium nitrate-modified titanium on *Pseudomonas aeruginosa* and *Staphylococcus aureus* biofilms formation. *J Biomater Tissue Eng.* 2017;7:743-747.
8. Giti R, Zomorodian K, Firouzmandi M, Zarehshahabadi Z, Rahmannasab S. Antimicrobial activity of thermocycled polymethyl methacrylate resin reinforced with titanium dioxide and copper oxide nanoparticles. *Int J Dent;* 2021.
9. Juan L, Zhimin Z, Anchun M, Lei L, Jingchao Z. Deposition of silver nanoparticles on titanium surface for antibacterial effect. *Int. J. Nanomedicine.* 2010;5:261–267.
10. Zhu Y, Qiu Y, Chen R, Liao L. The Inhibition of *Escherichia coli* biofilm formation by gallium nitrate-modified titanium. *J Nano Sci Nano technol.* 2015;15(8):5605–5609.
11. Antunes LCS, Imperi F, Minandri F, Visca P. *In Vitro* and *In Vivo* antimicrobial activities of gallium nitrate against multidrug-resistant *Acinetobacter baumannii*. *Antimicrob Agents and Chemother.* 2012;56(11):5961–5970.
12. Chitambar CR. The therapeutic potential of iron-targeting gallium compounds in human disease: From basic research to clinical application. *Pharmacol Res.* 2017;115:56-64.
13. Li F, Liu F, Huang K, Yang S. Advancement of gallium and gallium-based compounds as antimicrobial agents. *Front Bioeng Biotechnol.* 2022;10:827960.
14. Michalska K, Rychłowski M, Krupińska M, Szewczyk G, Sarna T, Nakonieczna J. Gallium mesoporphyrin IX-mediated photodestruction: a pharmacological trojan horse strategy to eliminate multidrug-resistant *Staphylococcus aureus*. *Mol Pharm.* 2022;19(5):1434-1448.
15. Tsukatani T, Suenaga H, Shiga M, Noguchi K, Ishiyama M, Ezoe T, et al. Comparison of the WST-8 colorimetric method and the CLSI broth microdilution method for susceptibility testing against drug-resistant bacteria. *J Microbiol Methods.* 2012;90(3):160-166.
16. Zhao Y, Frost RL, Yang J, Martens WN. Size and morphology control of gallium oxide hydroxide GaO(OH), Nano- to micro-sized particles by soft-chemistry route without surfactant. *J Phy Chem C.* 2008;112(10):3568-3579.
17. Ristić M, Popovic S, Musić. Application of sol-gel method in the synthesis of gallium (III)-oxide. *Mater Lett.* 2005;59(10):1227:1233.
18. Garcia RA, Tennent DJ, Chang D, Wenke JC, Sanchez Jr. CJ. An *In Vitro* comparison of PMMA and calcium sulfate as carriers for the local delivery of Gallium(III) nitrate to staphylococcal infected surgical sites. *Bio Med ResInt.* 2016;e7078989.
19. Dong J, YangY, Xiang B, Wang Z, Zhang Y, Huang Y. Study of the inhibitory effect of gallium nitrate-modified titanium on *Pseudomonas aeruginosa* and *Staphylococcus aureus* biofilms formation. *J Biomater Tissue Eng.* 2017;7:743-747.
20. Gugala N, Vu D, Parkins MD, Turner RJ. Specificity in the susceptibilities of *Escherichia coli*, *Pseudomonas aeruginosa* and *Staphylococcus aureus* clinical isolates to six metal antimicrobials. *Antibiotics.* 2019;8:51-63.
21. Best MG, Cunha-Reis C, Ganin AY, Sousa A, Johnston J, Oliveira AL, Smith DGE, Yiu

- HHP, Cooper IR. Antimicrobial properties of Gallium(III)- and Iron(III)-Loaded polysaccharides affecting the growth of *Escherichia coli*, *Staphylococcus aureus*, and *Pseudomonas aeruginosa*, *In vitro*. *ACS Appl Bio Mater*. 2020;3:7589-7597.
22. Rodríguez-Contreras A, Torres D, Guillem-Martí J, Sereno P, Ginebra MP, Calero JA, et al. Development of novel dual-action coatings with osteoinductive and antibacterial properties for 3D-printed titanium implants. *Surf Coat Technol*. 2020;403:126381.
23. Cochis A, Azzimonti B, Chiesa R, Rimondini L, Gasik M. Metallurgical gallium additions to titanium alloys demonstrate a strong time-increasing antibacterial activity without any cellular toxicity. *ACS Biomater Sci Eng*. 2019;5: 2815-2820.

© 2023 Assis et al.; This is an Open Access article distributed under the terms of the Creative Commons Attribution License (<http://creativecommons.org/licenses/by/4.0>), which permits unrestricted use, distribution, and reproduction in any medium, provided the original work is properly cited.

Peer-review history:

The peer review history for this paper can be accessed here:
<https://www.sdiarticle5.com/review-history/99020>